
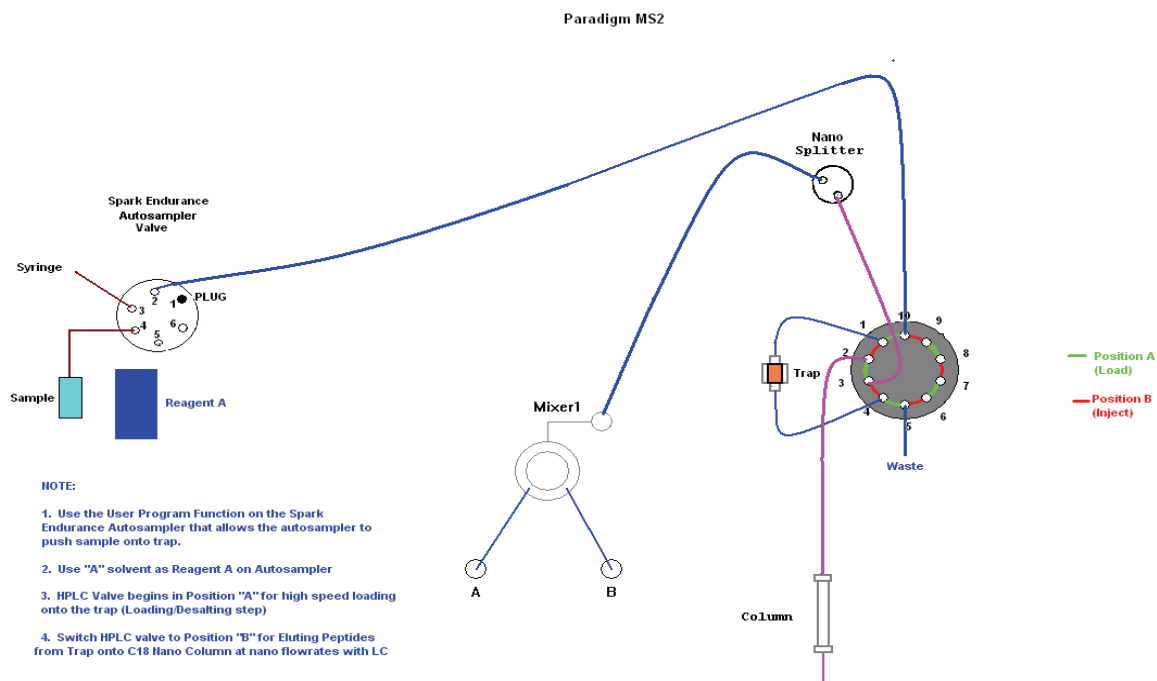


ul pickup with trapping method using the syringe to push the sample onto trap

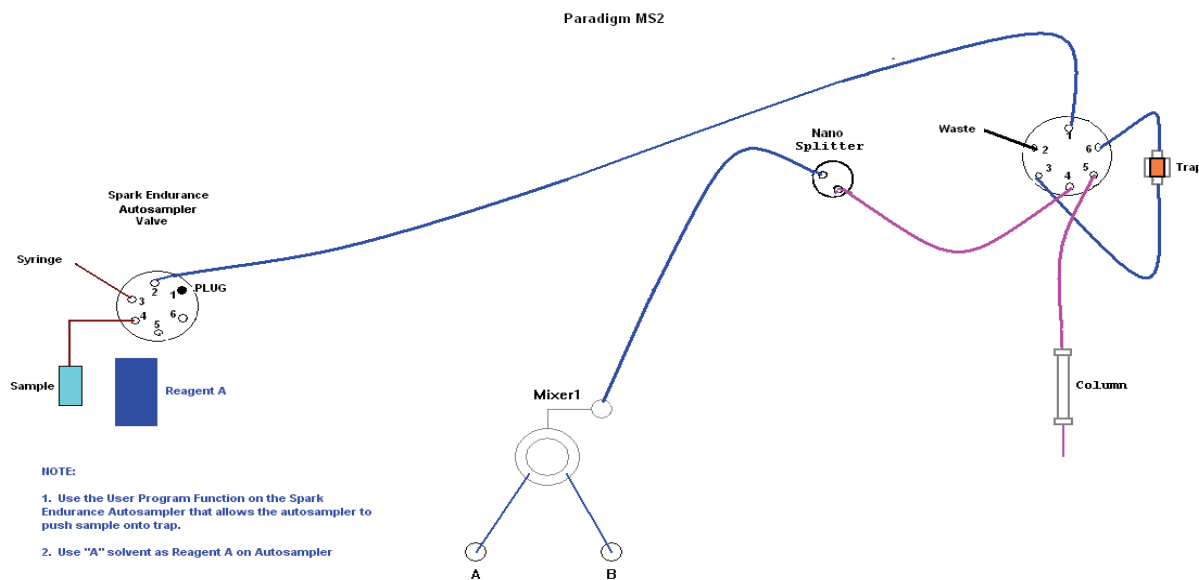

The top picture is for connecting to the divert valve on the Mass Spec while the bottom picture is for connecting to the Paradigm. Each of these will use the trapping method in User program.